# How to download AgenT 5.x

## 1) from the Zeppelin page entered via InCenter access:

http://pww.zeppelin.philips.com/zeppelin/user/toolbox.asp

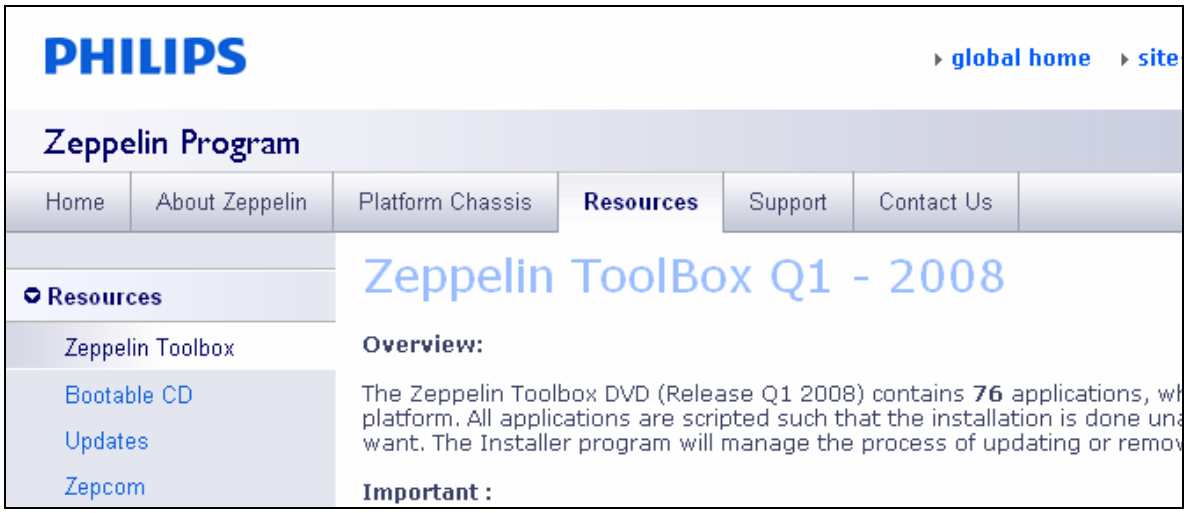


**Zeppelin Extended ToolBox**

| # | Application Name | Modality | Download Link for Windows 2000 | Download Link for Windows XP |
|---|---|---|---|---|
| 24 | ACCO Print Spooler 1.0 | X-ray | Download (1,945 KB) | Download (1,945 KB) |
| 25 | AGent 5.1 | X-ray | Download (12,904 KB) | Download (12,904 KB) |

## 2) from the Intranet Service Library page:

http://incenter.medical.philips.com/default.aspx

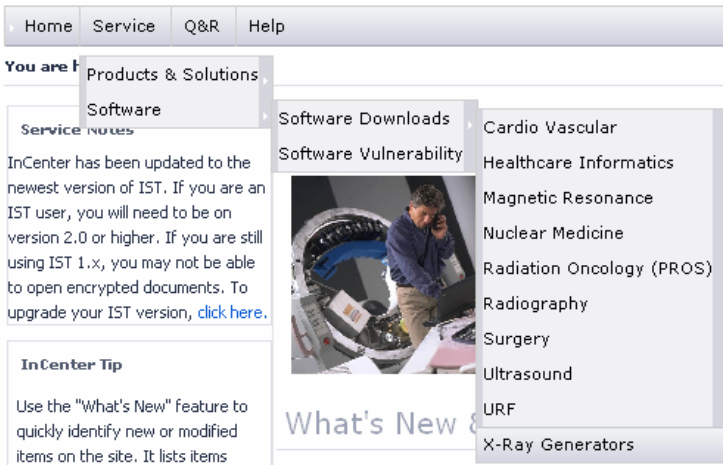
Home
Service
Q&R
Help
You are h
Products & Solutions
Software
Service Notes
InCenter has been updated to the newest version of IST. If you are an IST user, you will need to be on version 2.0 or higher. If you are still using IST 1.x, you may not be able to open encrypted documents. To upgrade your IST version, click here.
InCenter Tip
Use the "What's New" feature to quickly identify new or modified items on the site. It lists items
Software Downloads
Software Vulnerability
What's New &
Cardio Vascular
Healthcare Informatics
Magnetic Resonance
Nuclear Medicine
Radiation Oncology (PROS)
Radiography
Surgery
Ultrasound
URF
X-Ray Generators

Select either **OPTIMUS RAD/RF** or **Velara** and **Other Downloads** >> **AGenT_5x.zip**.

AgenT 5.x can be used for all generators Optimus RAD release 2.3, Optimus RAD+RF release 3.x, Optimus C release 1.x, Optimus CXA and all versions Velara.

Additional information for the use of AgenT (in comparison with XRGSCOPE for Optimus RAD-R/F-C) can be loaded from the download area Optimus, select the blue marked items.

The **PC <=> device** communication can be improved with the information on the next pages.

Measures to increase the safe backup / restore of data with AgenT, especially for CU backup procedures (running on mains will not interrupt the communication):

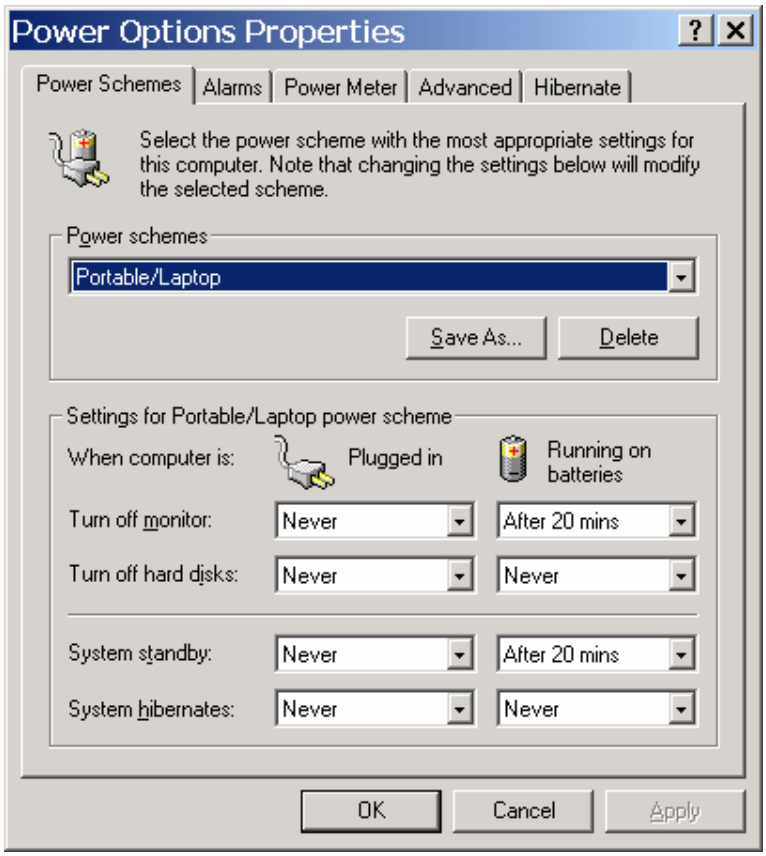


Serial Port settings:




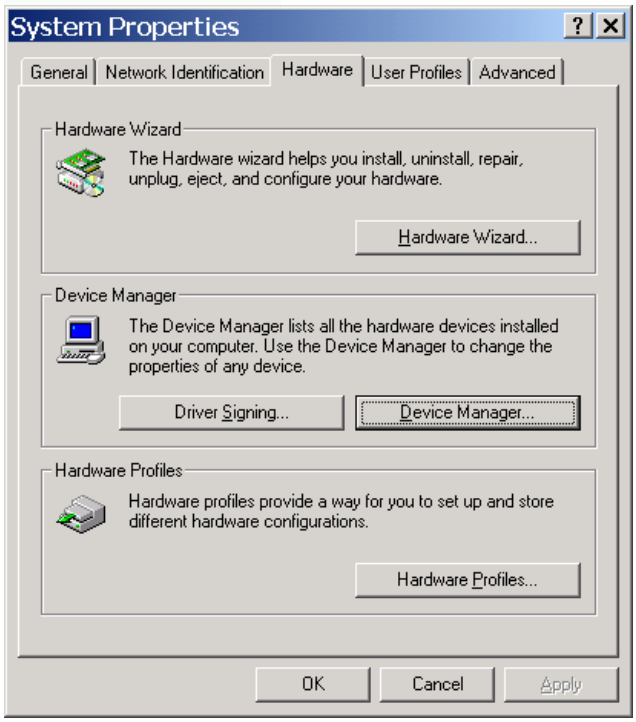
System Properties
General
Network Identification
Hardware
User Profiles
Advanced
Hardware Wizard
The Hardware wizard helps you install, uninstall, repair, unplug, eject, and configure your hardware.
Hardware Wizard...
Device Manager
The Device Manager lists all the hardware devices installed on your computer. Use the Device Manager to change the properties of any device.
Driver Signing...
Device Manager...
Hardware Profiles
Hardware profiles provide a way for you to set up and store different hardware configurations.
Hardware Profiles...
OK
Cancel
Apply

Select Device Manager

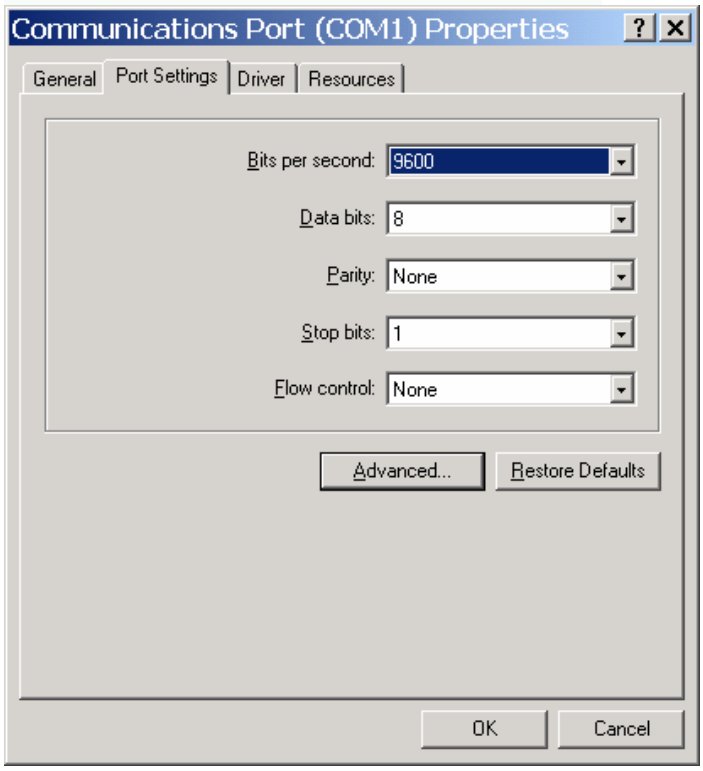


Select Advanced

Change Advanced Settings from High to Low:

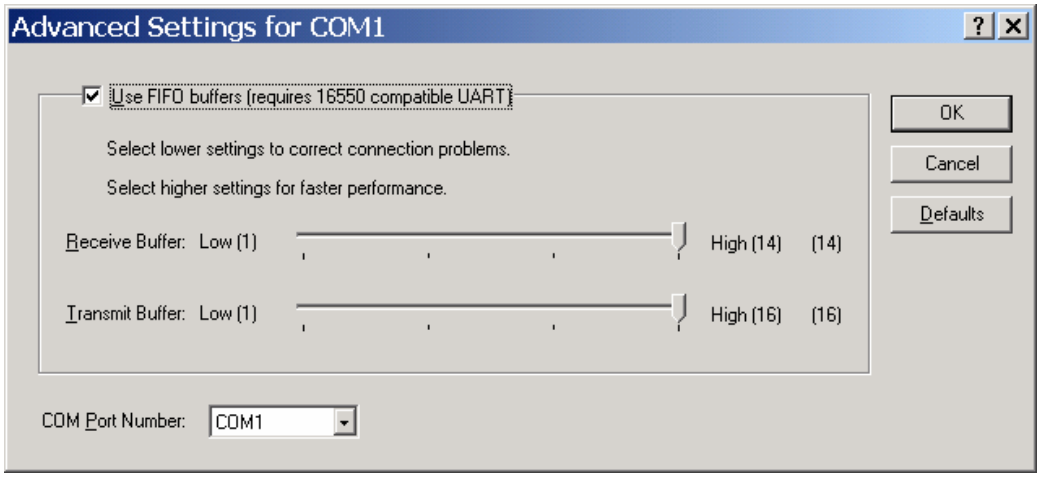
Advanced Settings for COM1
Use FIFO buffers (requires 16550 compatible UART)
Select lower settings to correct connection problems.
Select higher settings for faster performance.
Receive Buffer: Low (1) High (14) (14)
Transmit Buffer: Low (1) High (16) (16)
COM Port Number: COM1
OK
Cancel
Defaults

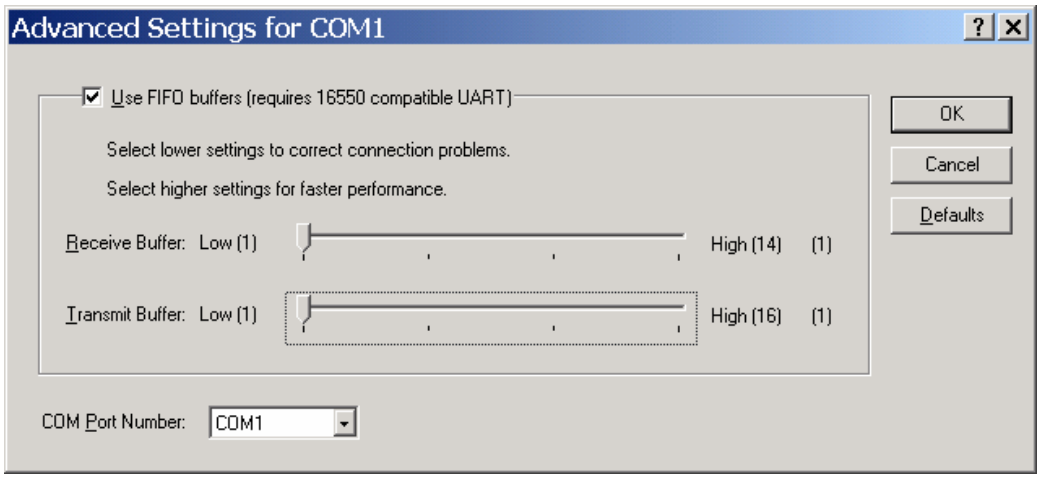
Advanced Settings for COM1
Use FIFO buffers (requires 16550 compatible UART)
Select lower settings to correct connection problems.
Select higher settings for faster performance.
Receive Buffer: Low (1) High (14) (1)
Transmit Buffer: Low (1) High (16) (1)
COM Port Number: COM1
OK
Cancel
Defaults